

Adapting to OLYMPUS 140 Series Immersible Endoscopes**


If ordering adapters:



NOTE: the ends of the adapters shown plug into the manifold.



If your machine is equipped with this type of end add an "M" when reordering adapter. e.g.: 16002M or 16006M

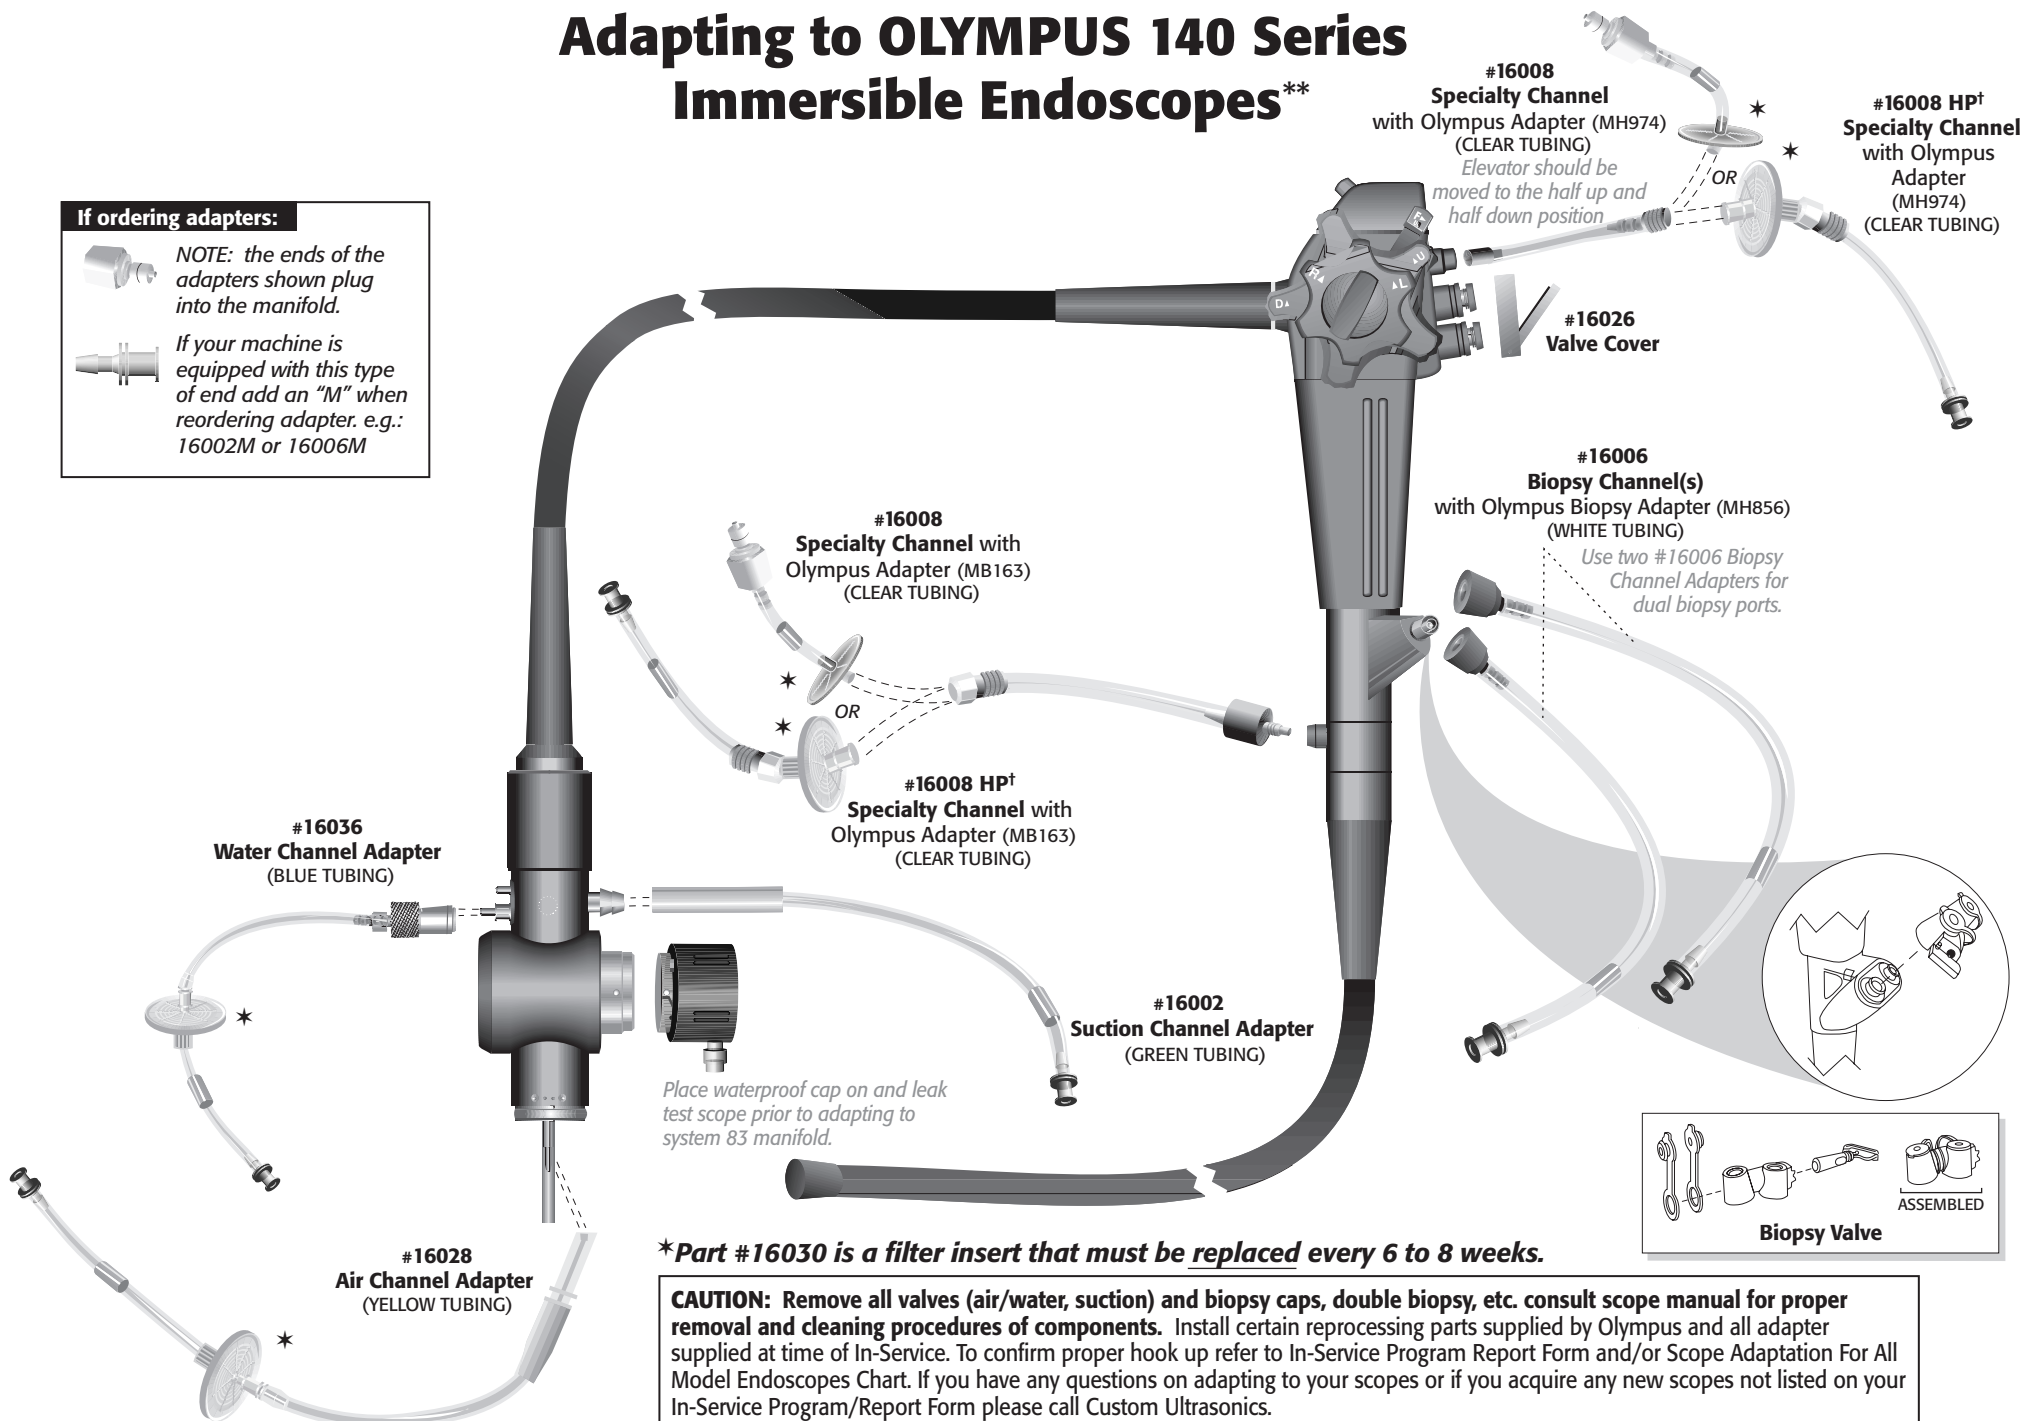

** This adapter chart for Olympus Flexible Endoscopes illustrates various models and does not represent an actual model.

† For machines that are equipped with High Pressure Ports use #16008 HP Specialty Channel.